

SEA-BIRD ELECTRONICS, INC.

13431 NE 20th Street, Bellevue, Washington, 98005-2010 USA

Phone: (425) 643 - 9866 Fax (425) 643 - 9954 Email: seabird@seabird.com

SENSOR SERIAL NUMBER: 0131
CALIBRATION DATE: 25-Jul-11

GliderAPL TEMPERATURE CALIBRATION DATA
ITS-90 TEMPERATURE SCALE

ITS-90 COEFFICIENTS

g = 4.35541220e-003
h = 6.23233378e-004
i = 2.23747165e-005
j = 2.26794066e-006
f0 = 1000.0

IPTS-68 COEFFICIENTS

a = 3.64763863e-003
b = 5.80051563e-004
c = 1.43741110e-005
d = 2.26932222e-006
f0 = 3253.158

BATH TEMP (ITS-90)	INSTRUMENT FREQ (Hz)	INST TEMP (ITS-90)	RESIDUAL (ITS-90)
0.9999	3253.158	0.9997	-0.00018
4.4999	3522.185	4.5002	0.00031
14.9999	4425.852	14.9998	-0.00008
18.5000	4760.812	18.4997	-0.00029
24.0000	5322.926	24.0001	0.00012
29.0000	5872.936	29.0004	0.00040
32.5000	6280.565	32.4997	-0.00027

Temperature ITS-90 = $1/\{g + h[\ln(f_0/f)] + i[\ln^2(f_0/f)] + j[\ln^3(f_0/f)]\} - 273.15$ (°C)


Temperature IPTS-68 = $1/\{a + b[\ln(f_0/f)] + c[\ln^2(f_0/f)] + d[\ln^3(f_0/f)]\} - 273.15$ (°C)

Following the recommendation of JPOTS: T_{68} is assumed to be $1.00024 * T_{90}$ (-2 to 35 °C)

Residual = instrument temperature - bath temperature

Date, Offset(mdeg C)

● 23-Oct-09 -5.36
▲ 25-Jul-11 -0.00

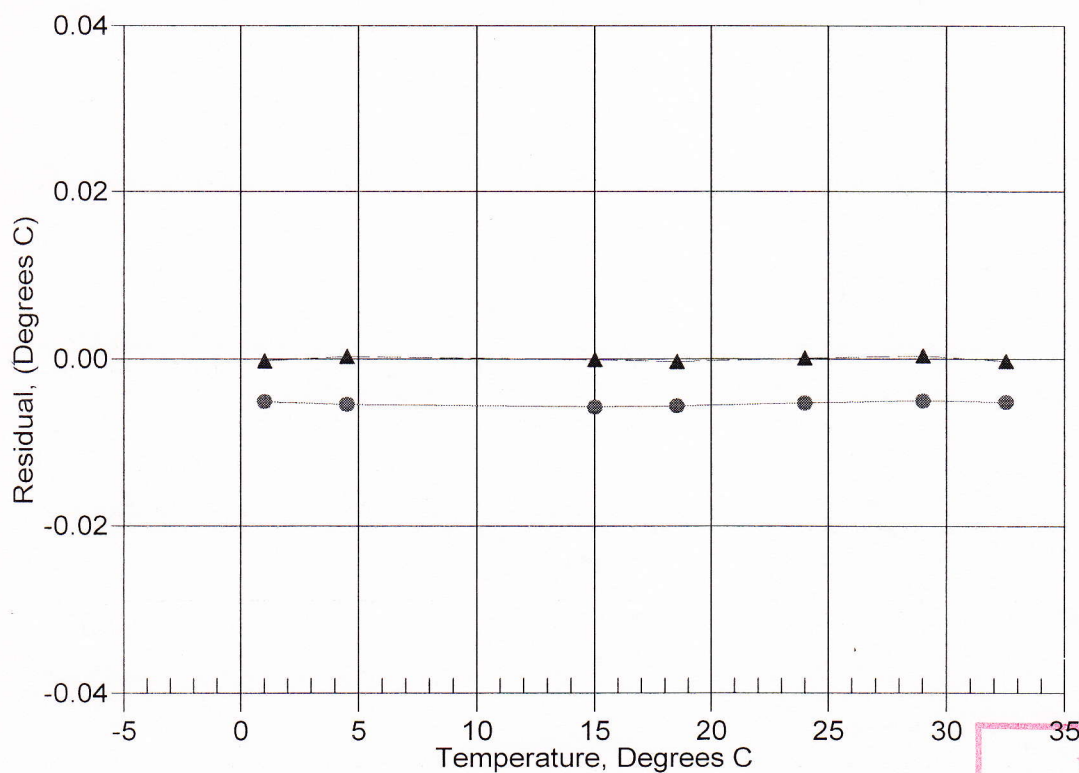

POST CRUISE
CALIBRATION

SEA-BIRD ELECTRONICS, INC.

13431 NE 20th Street, Bellevue, Washington, 98005-2010 USA

Phone: (425) 643 - 9866 Fax (425) 643 - 9954 Email: seabird@seabird.com

SENSOR SERIAL NUMBER: 0131
CALIBRATION DATE: 25-Jul-11

GliderAPL CONDUCTIVITY CALIBRATION DATA
PSS 1978: C(35,15,0) = 4.2914 Siemens/meter

GHJ COEFFICIENTS

g = -1.01065236e+001
h = 1.13245203e+000
i = -2.43355714e-003
j = 2.73086662e-004
CPcor = -9.5700e-008 (nominal)
CTcor = 3.2500e-006 (nominal)

ABCDM COEFFICIENTS

a = 5.09697910e-006
b = 1.12518834e+000
c = -1.00842916e+001
d = -8.84905051e-005
m = 5.3
CPcor = -9.5700e-008 (nominal)

BATH TEMP (ITS-90)	BATH SAL (PSU)	BATH COND (Siemens/m)	INST FREQ (kHz)	INST COND (Siemens/m)	RESIDUAL (Siemens/m)
22.0000	0.0000	0.00000	2.99378	0.00000	0.00000
0.9999	34.8106	2.97552	5.94558	2.97552	0.00001
4.4999	34.7911	3.28257	6.16981	3.28257	-0.00000
14.9999	34.7484	4.26415	6.83668	4.26414	-0.00001
18.5000	34.7393	4.60926	7.05589	4.60926	0.00000
24.0000	34.7293	5.16711	7.39619	5.16712	0.00001
29.0000	34.7240	5.68890	7.70051	5.68891	0.00001
32.5000	34.7212	6.06128	7.91031	6.06127	-0.00001


Conductivity = $(g + hf^2 + if^3 + jf^4) / 10(1 + \delta t + \epsilon p)$ Siemens/meter

Conductivity = $(af^m + bf^2 + c + dt) / [10(1 + \epsilon p)]$ Siemens/meter

t = temperature[°C]; p = pressure[decibars]; δ = CTcor; ϵ = CPcor;

Residual = (instrument conductivity - bath conductivity) using g, h, i, j coefficients

Date, Slope Correction

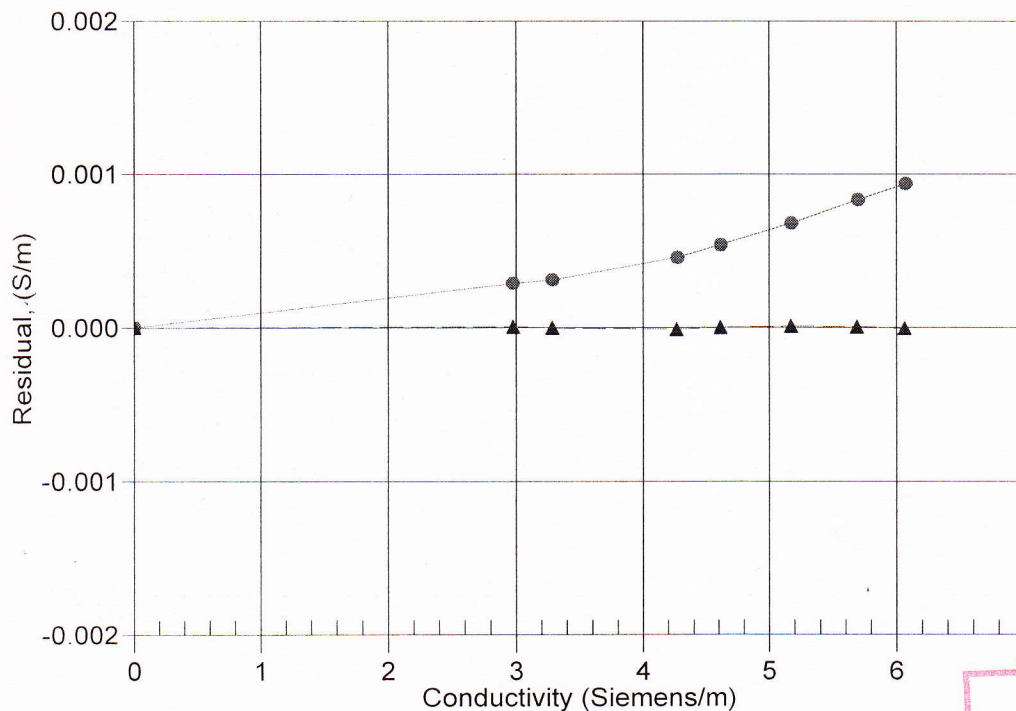

● 23-Oct-09 0.9998692
▲ 25-Jul-11 1.0000000

POST CRUISE
CALIBRATION



SEA-BIRD ELECTRONICS, INC.

13431 NE 20th Street Bellevue, Washington 98005 USA

Phone: (425) 643-9866 Fax: (425) 643-9954 www.seabird.com

Conductivity Calibration Report

Customer:	Lockheed Martin		
Job Number:	65316	Date of Report:	7/25/2011
Model Number:	Glider	Serial Number:	0131 Glider

Conductivity sensors are normally calibrated 'as received', without cleaning or adjustments, allowing a determination of sensor drift. If the calibration identifies a problem or indicates cell cleaning is necessary, then a second calibration is performed after work is completed. The 'as received' calibration is not performed if the sensor is damaged or non-functional, or by customer request.

An 'as received' calibration certificate is provided, listing the coefficients used to convert sensor frequency to conductivity. Users must choose whether the 'as received' calibration or the previous calibration better represents the sensor condition during deployment. In SEASOFT enter the chosen coefficients using the program SEACON. The coefficient 'slope' allows small corrections for drift between calibrations (consult the SEASOFT manual). Calibration coefficients obtained after a repair or cleaning apply only to subsequent data.

'AS RECEIVED CALIBRATION'

☒ Performed ☐ Not Performed

Date: 7/25/2011

Drift since last cal: -0.00020 PSU/month*

Comments:

'CALIBRATION AFTER CLEANING & REPLATINIZING'

☐ Performed ☒ Not Performed

Date:

Drift since Last cal: PSU/month*

Comments:

*Measured at 3.0 S/m

Cell cleaning and electrode replatinizing tend to 'reset' the conductivity sensor to its original condition. Lack of drift in post-cleaning-calibration indicates geometric stability of the cell and electrical stability of the sensor circuit.

SBE SEA-BIRD ELECTRONICS, INC.

13431 NE 20th St. Bellevue, Washington 98005 USA



Phone: (425) 643-9866 Fax: (425) 643-9954 www.seabird.com

Service

Report

RMA Number

65316

Customer Information:

Company Lockheed Martin

Date 7/26/2011

Contact Domenic Jannarelli

PO Number TBD

Serial Number 0131 Glider

Model Number Glider

Services Requested:

1. Evaluate/Repair Instrumentation.
2. Perform Routine Calibration Service.

Problems Found:

Services Performed:

1. Performed initial diagnostic evaluation.
2. Performed "Post Cruise" calibration of the temperature & conductivity sensors.
3. Performed complete system check and full diagnostic evaluation.

Special Notes:



SEA-BIRD ELECTRONICS, INC.

13431 NE 20th St. Bellevue, Washington 98005 USA

Phone: (425) 643-9866 Fax: (425) 643-9954 www.seabird.com

Temperature Calibration Report

Customer:	Lockheed Martin		
Job Number:	65316	Date of Report:	7/25/2011
Model Number:	Glider	Serial Number:	0131 Glider

Temperature sensors are normally calibrated 'as received', without adjustments, allowing a determination sensor drift. If the calibration identifies a problem, then a second calibration is performed after work is completed. The 'as received' calibration is not performed if the sensor is damaged or non-functional, or by customer request.

An 'as received' calibration certificate is provided, listing coefficients to convert sensor frequency to temperature. Users must choose whether the 'as received' calibration or the previous calibration better represents the sensor condition during deployment. In SEASOFT enter the chosen coefficients using the program SEACON. The coefficient 'offset' allows a small correction for drift between calibrations (consult the SEASOFT manual). Calibration coefficients obtained after a repair apply only to subsequent data.

'AS RECEIVED CALIBRATION'

☒ Performed ☐ Not Performed

Date: 7/25/2011

Drift since last cal: +0.00306 Degrees Celsius/year

Comments:

'CALIBRATION AFTER REPAIR'

☐ Performed ☒ Not Performed

Date:

Drift since Last cal: Degrees Celsius/year

Comments: